

Fig. 1

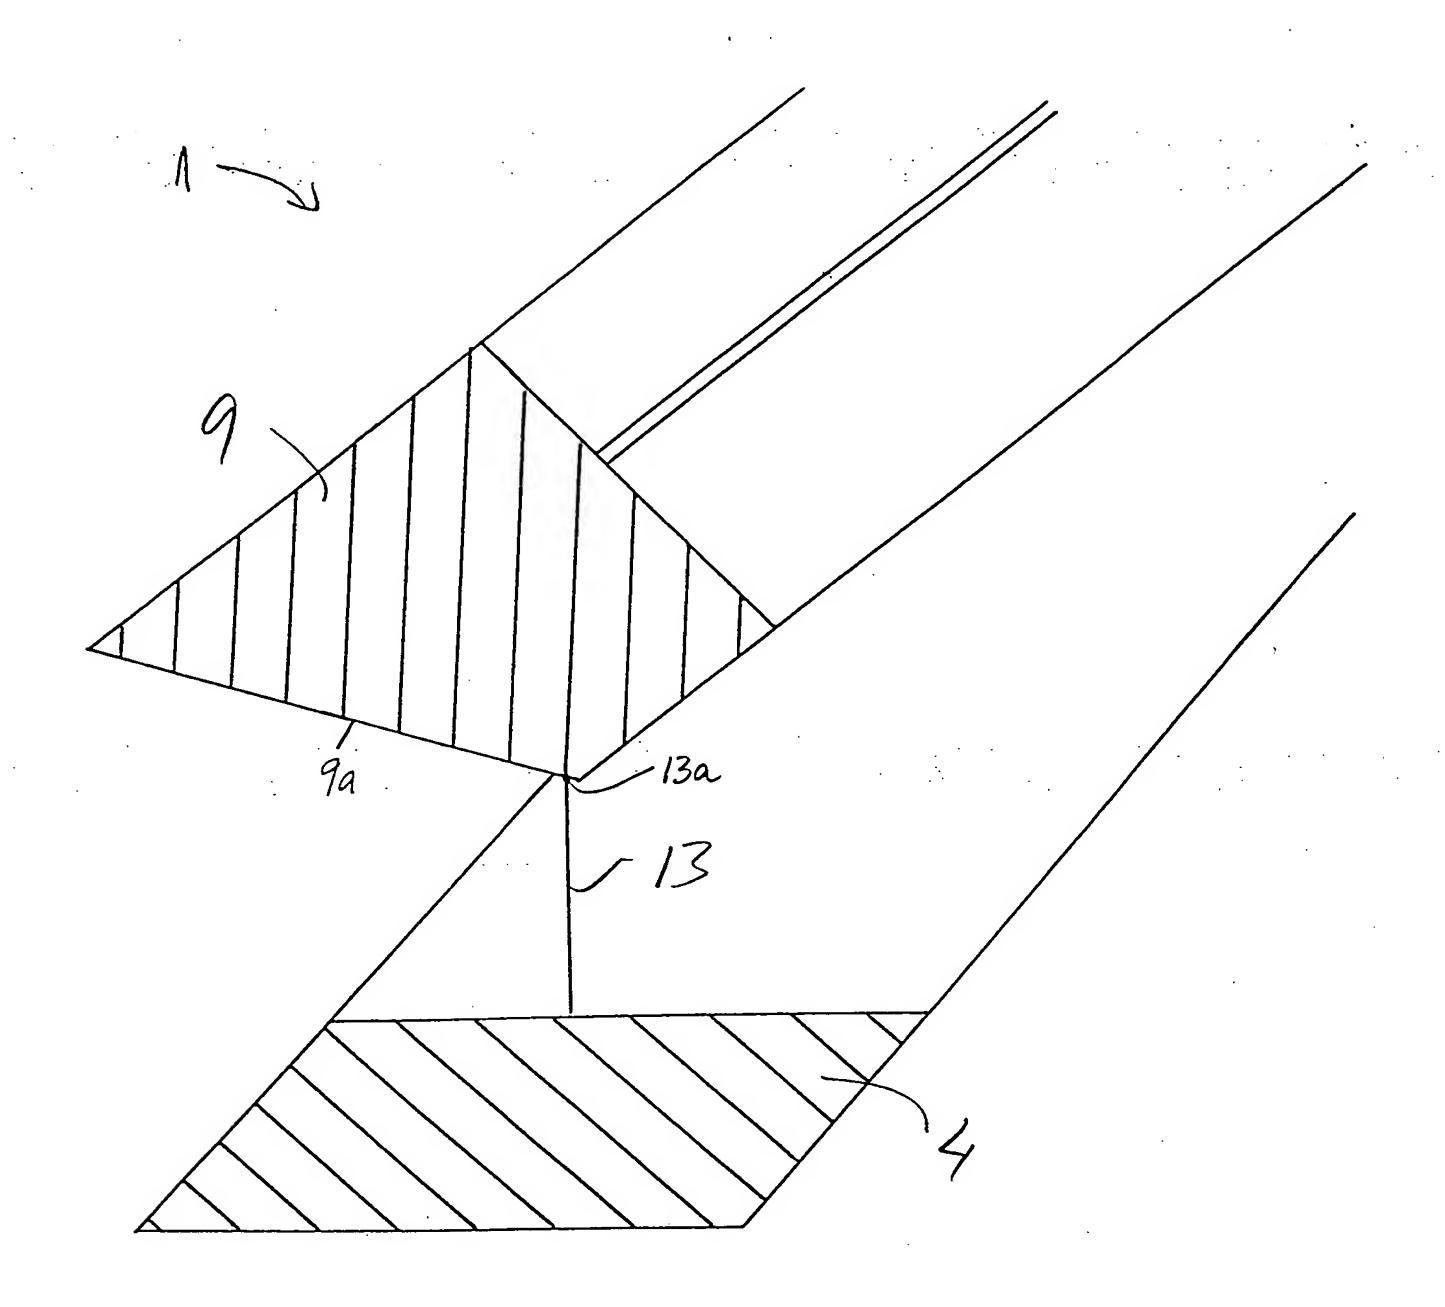


Fig. 2

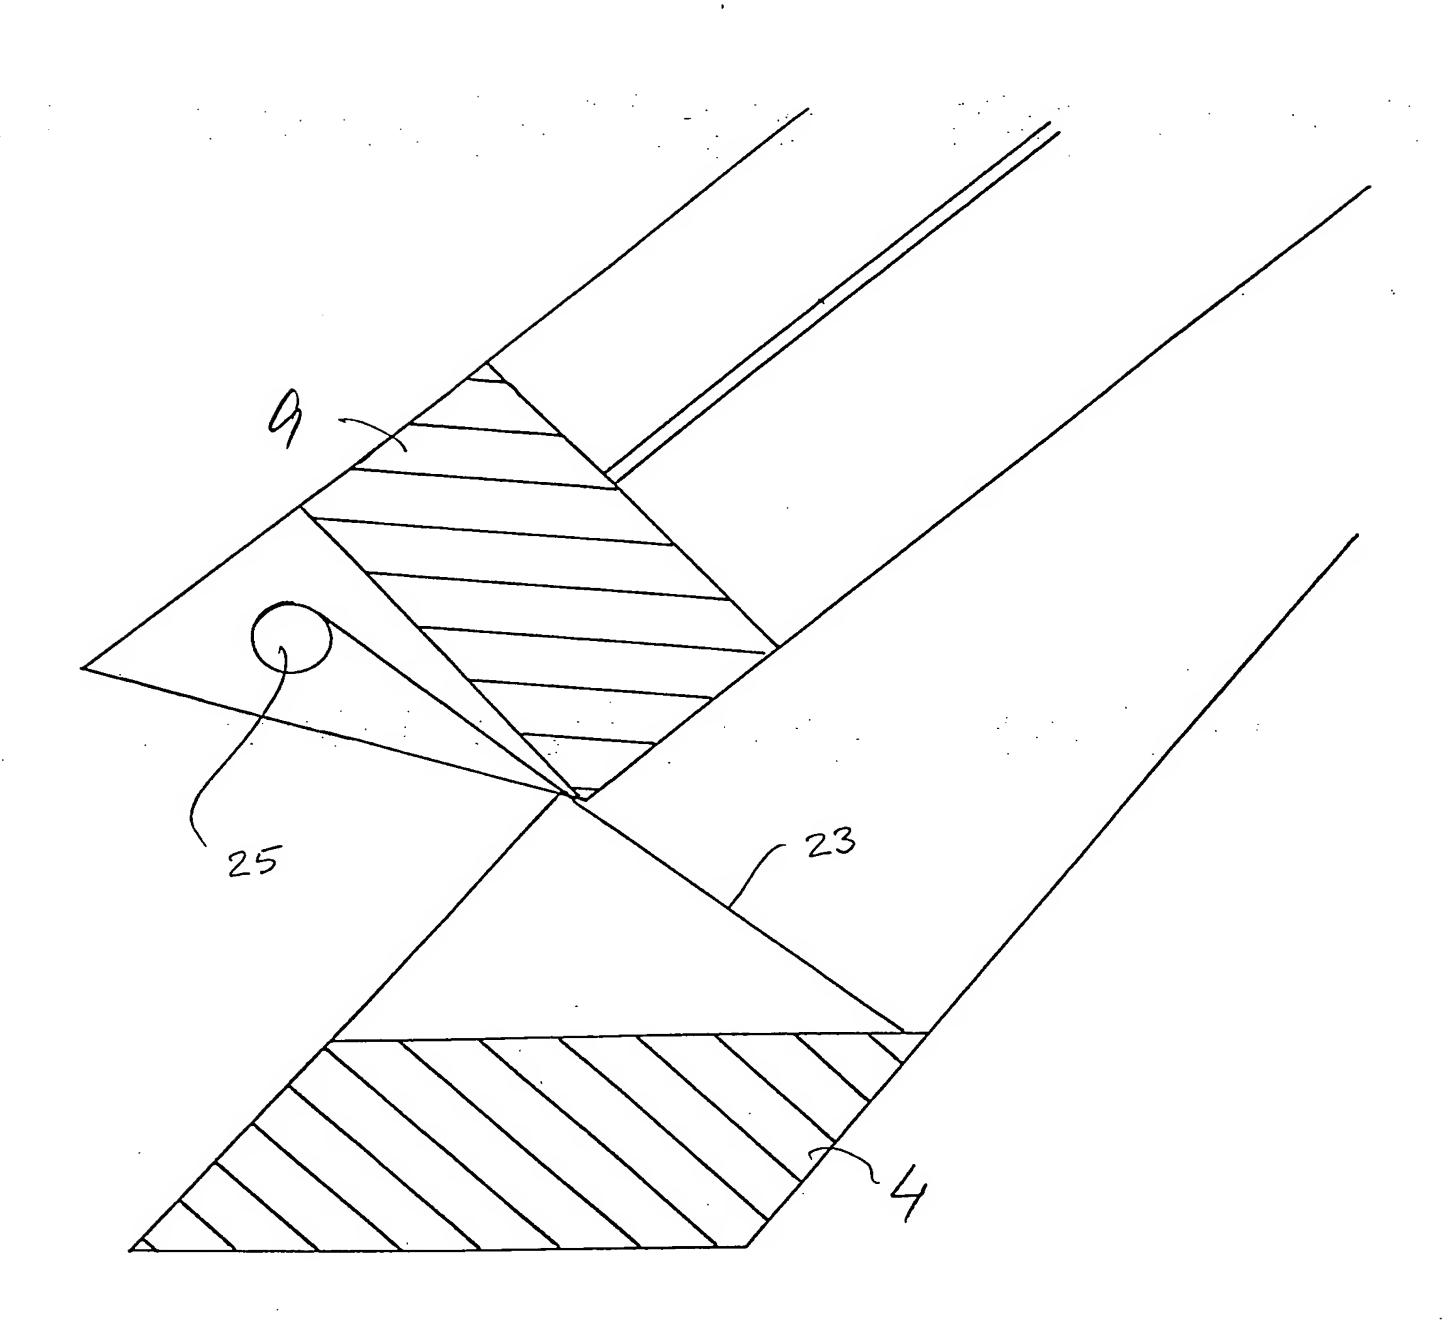


Fig. 3

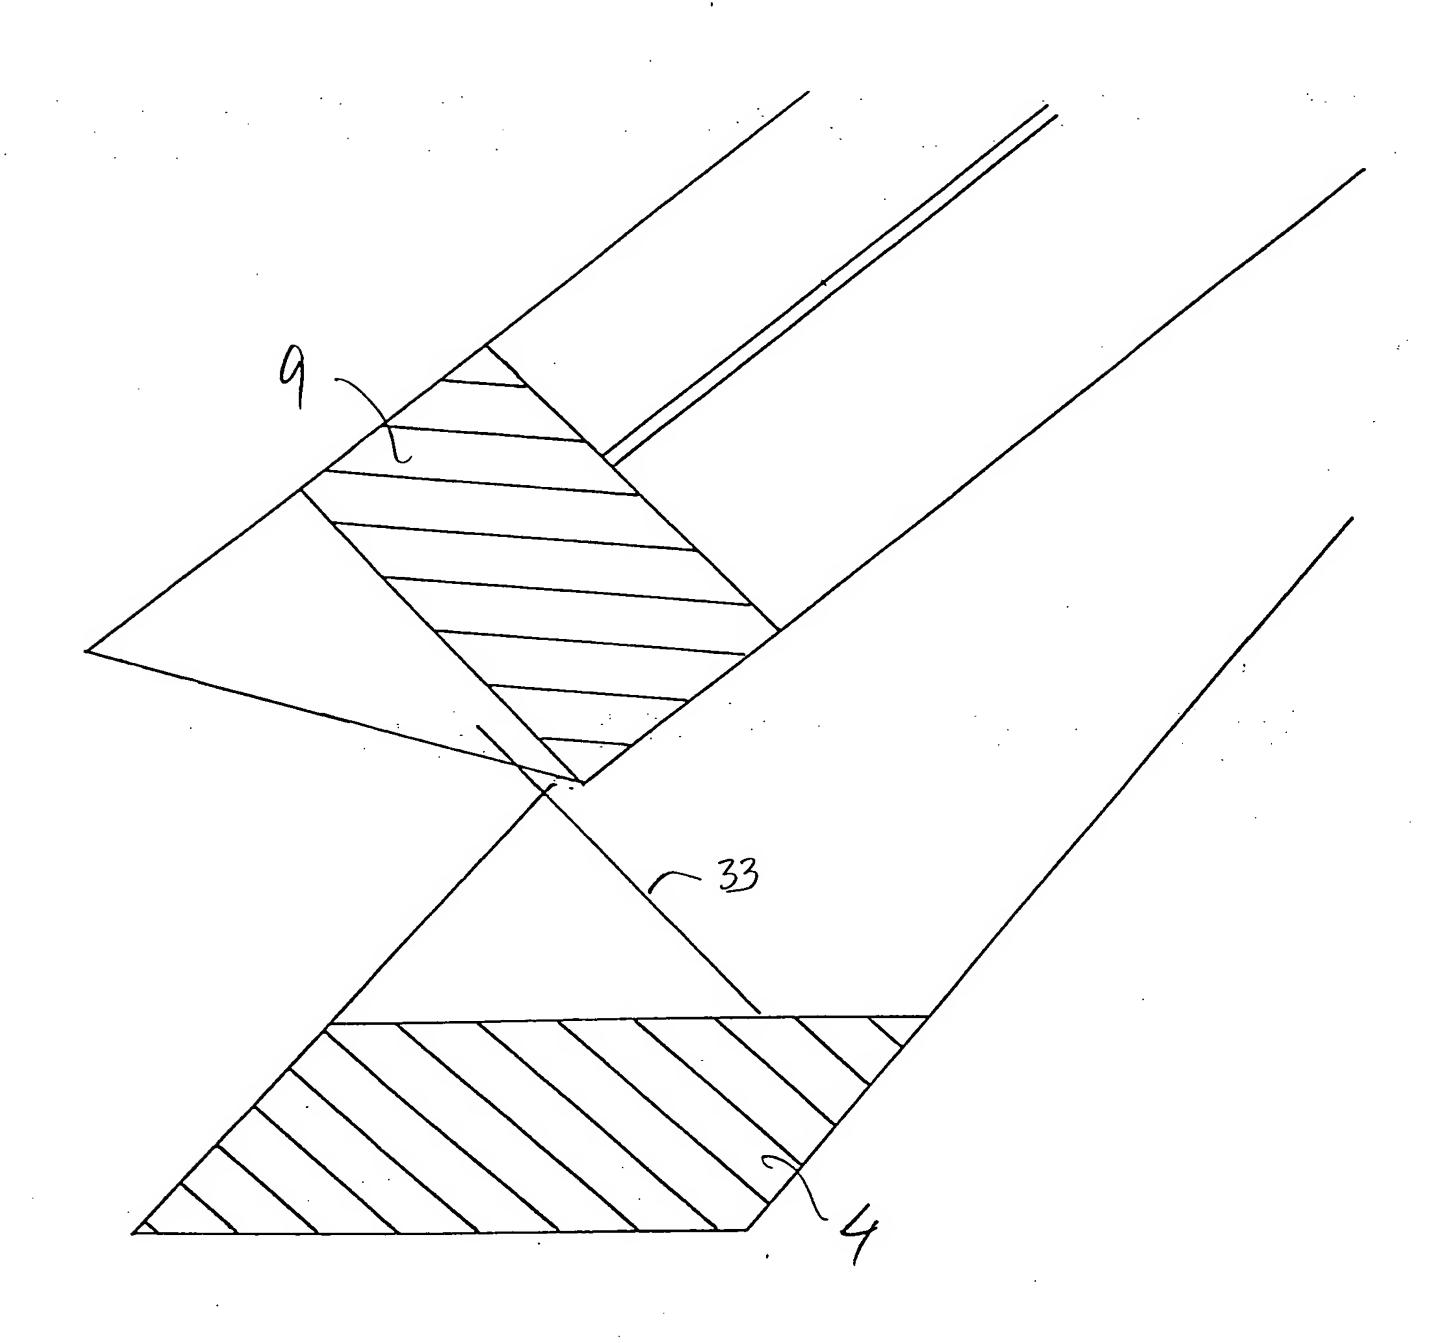


Fig. 4

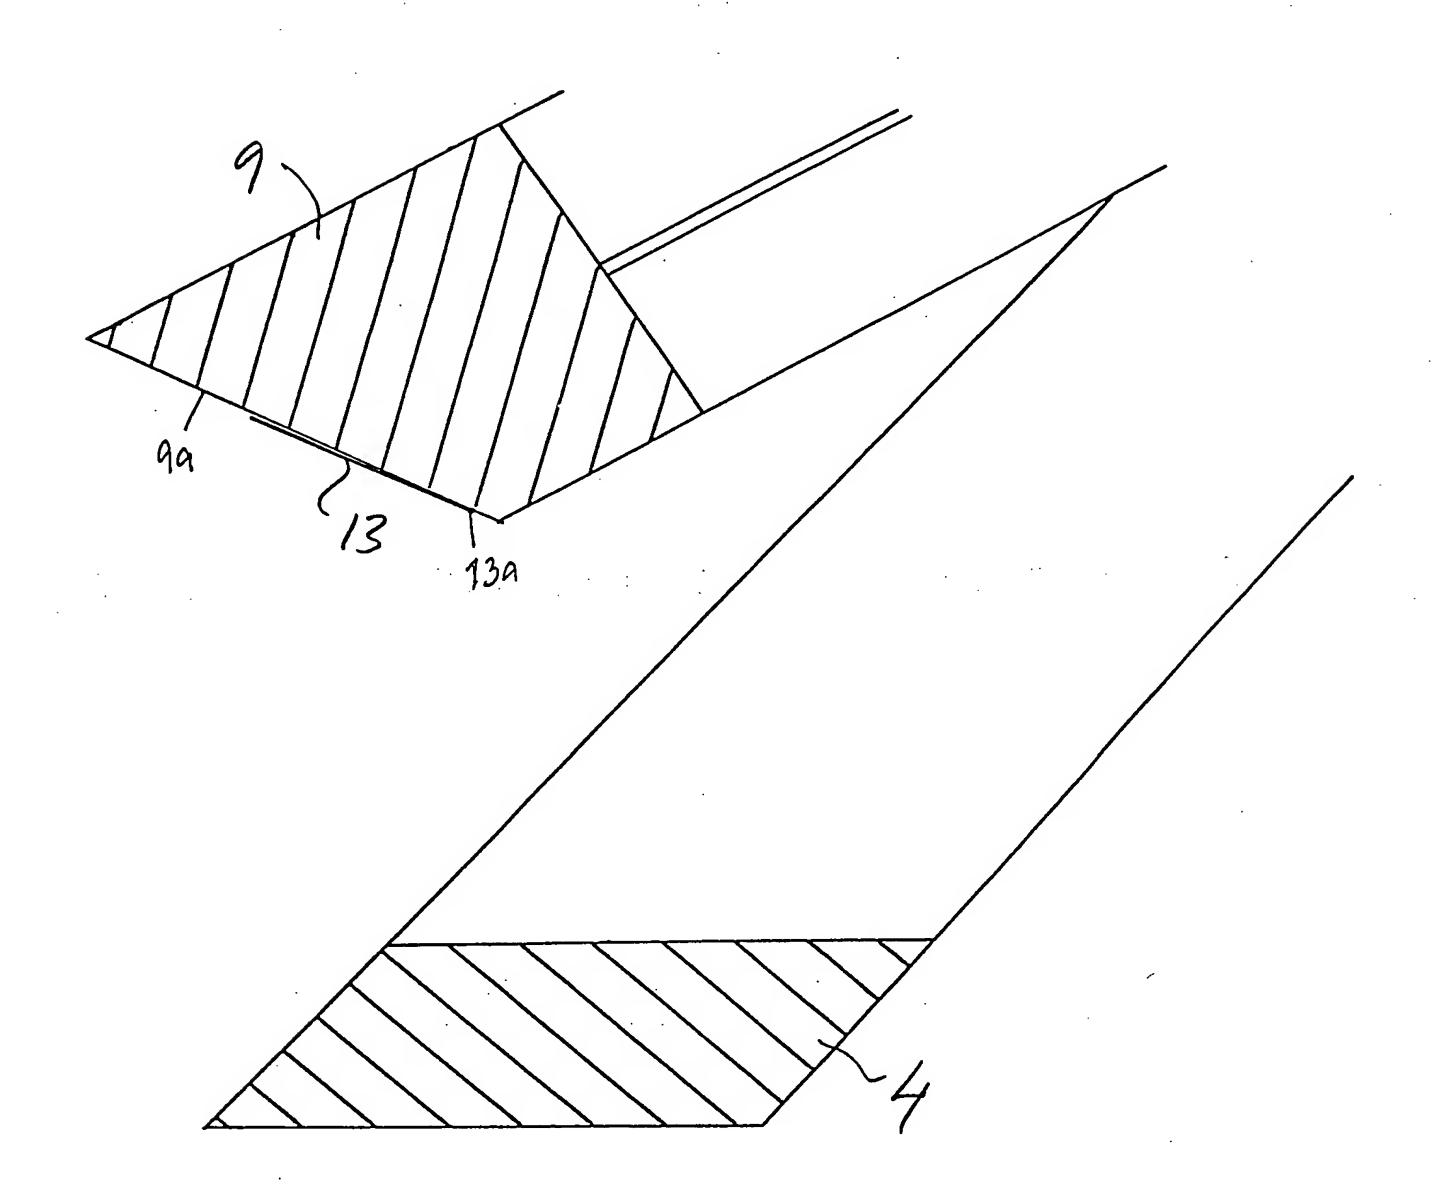


Fig. 5

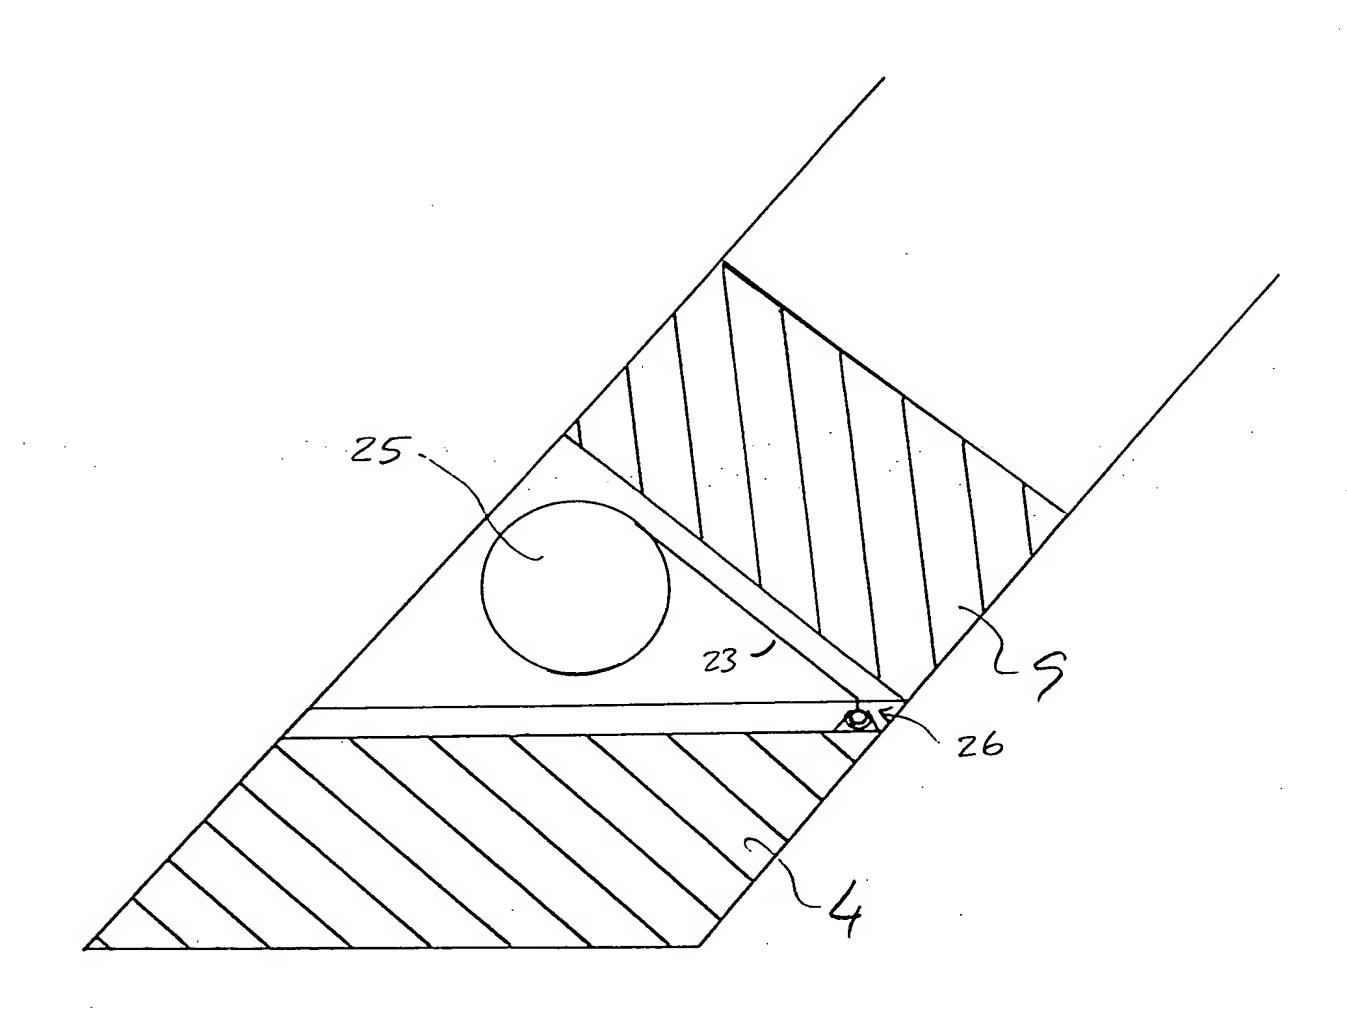
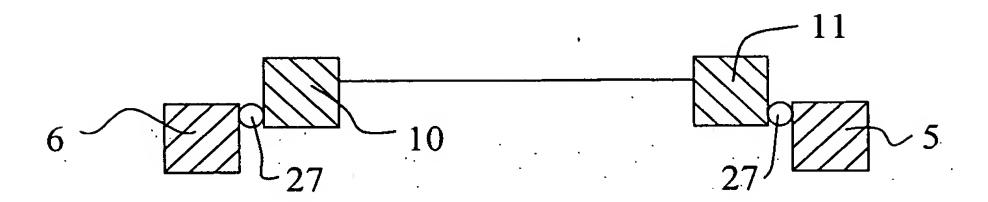
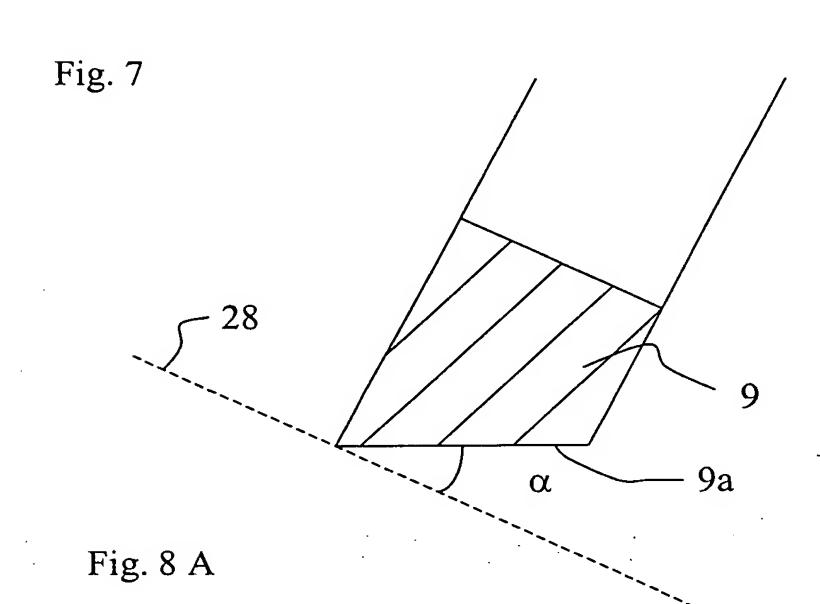


Fig. 6

## WINDOW WITH SCREENING ARRANGEMENT PER JACOBSEN PCT/DK2004/000469 7/9





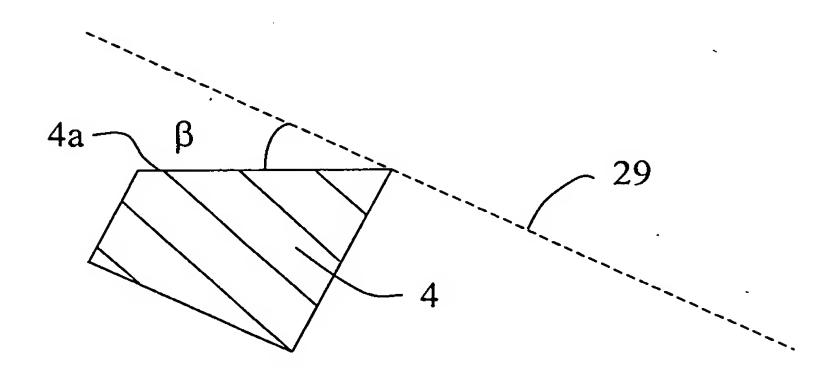


Fig. 8 B

## WINDOW WITH SCREENING ARRANGEMENT PER JACOBSEN PCT/DK2004/000469 8/9

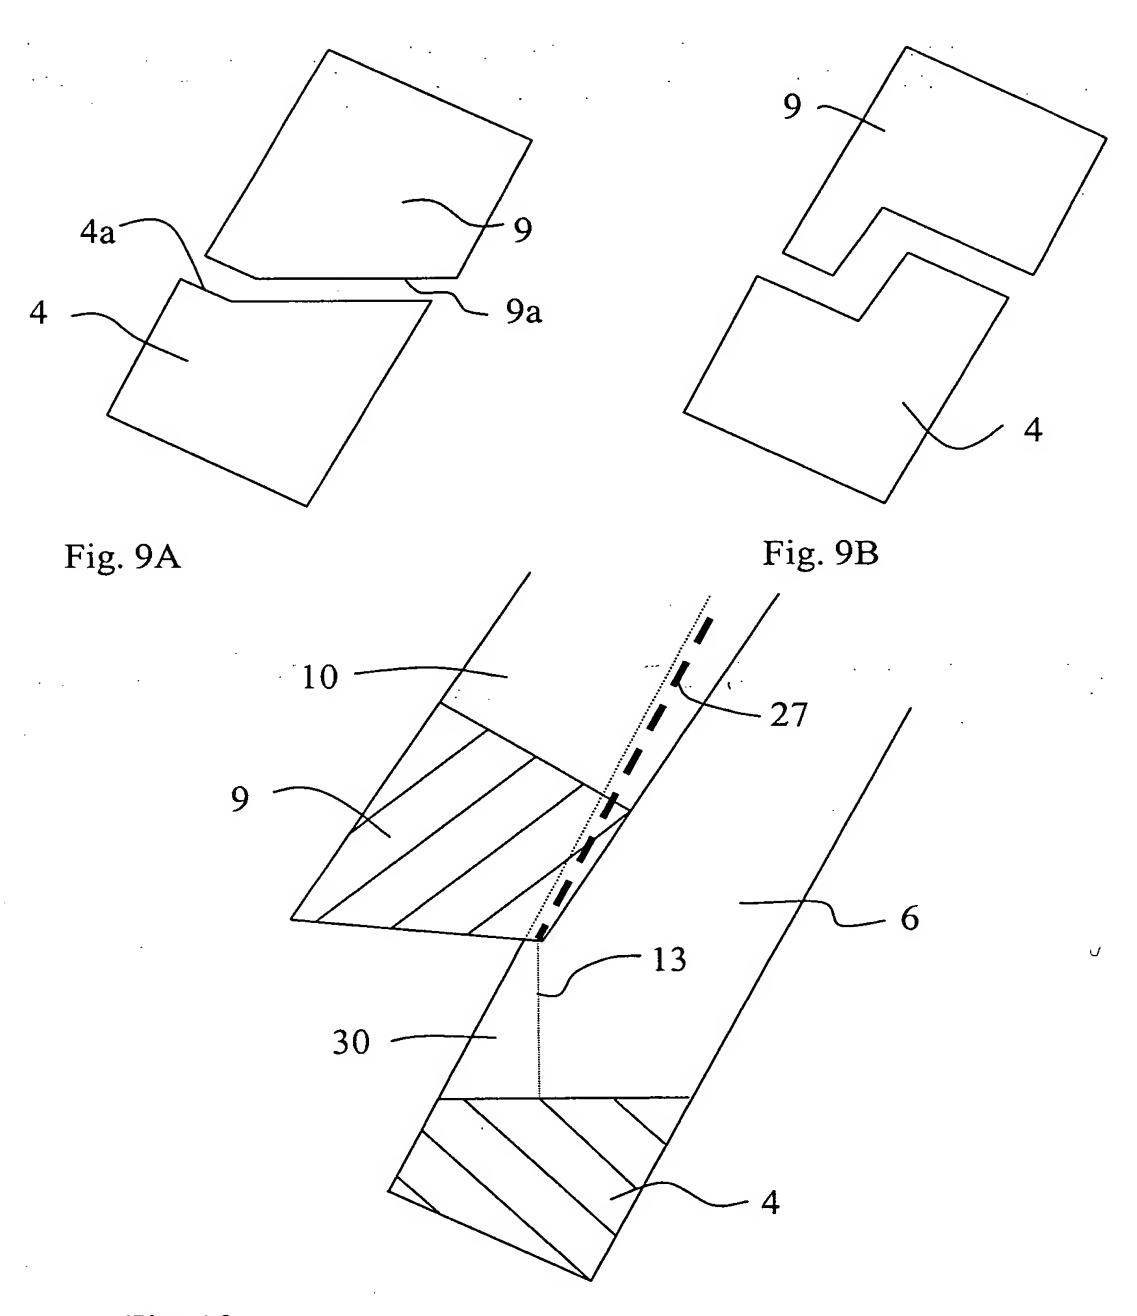


Fig. 10

